

Gima S.p.A.
Via Marconi, 1 - 20060 Gessate (MI) Italy
gima@gimaitaly.com - export@gimaitaly.com - **www.gimaitaly.com**

REF **20520 - 20521 - 20522 - 20529**
20531 - 20532 - 20533

Gima S.p.A.
Via Marconi, 1
20060 Gessate (MI) Italy
Made in Pakistan

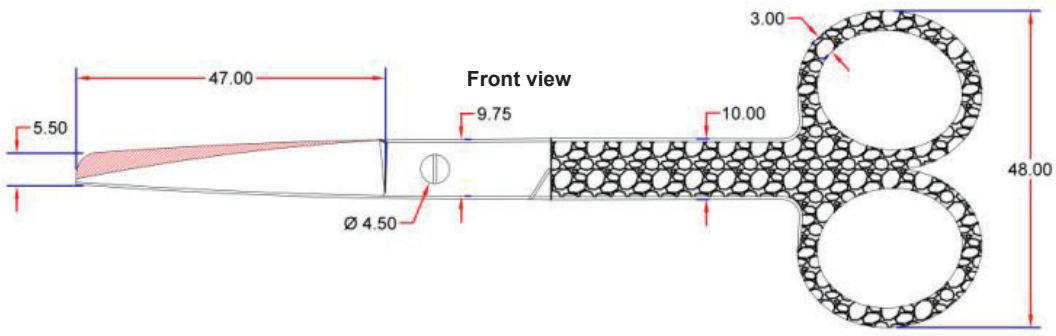

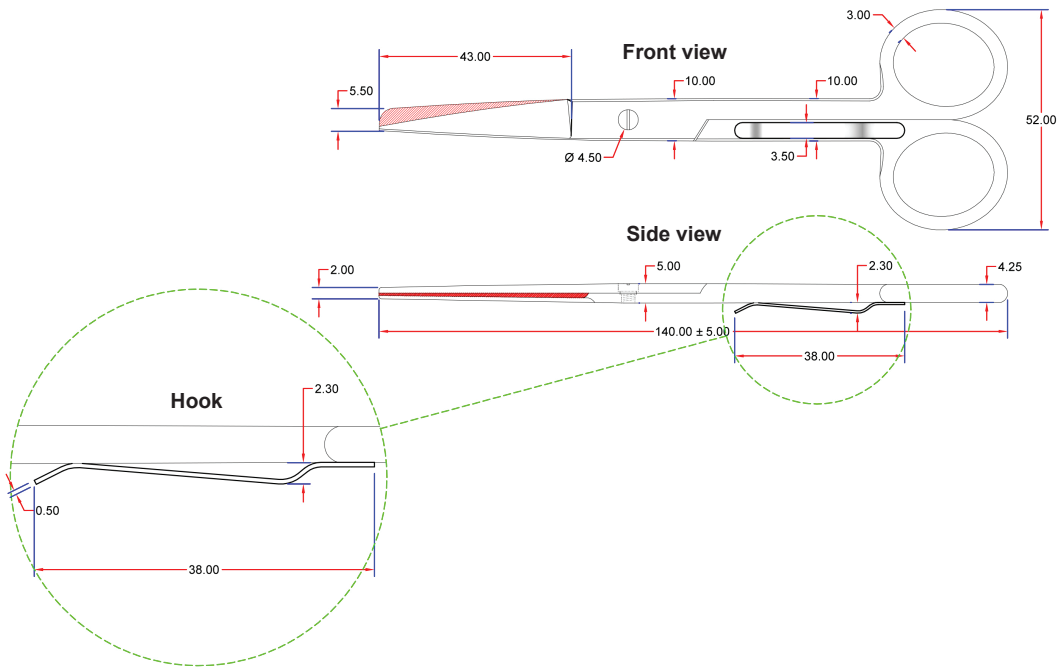

SURGICAL SCISSORS

ENGLISH

Detailed Description of the Device
Name: Surgical scissors SH/BL 14cm & Surgical scissors SH/BL 14cm with hook.
Finish: Satin & Powder Coating.

Instructions of Use
Surgical scissors are made of stainless steel type AISI-410 under standard ASTM F-899-84. They are used for cutting purpose.

Contents or Composition
ASTM Standard F-899-84

Carbon: 0,126%	Manganese: 0,514%	Phosphorus: 0,021%	Sulphur: 0,015%
Silicon: 0,275% max	Chromium: 13,503%	Nickel: 0,101%	

Indication of Use

- *Put away from the reach of uncontrolled person.*
- *A trained person shall use the devices.*
- *Do not sterilize the instruments with a solution with Chloride ions. Sterilization solution shall have a pH near to 6.0 - 7.0.*
- *For professional use only – disinfect before use.*

Precautions, restrictions, warnings, special cares

Methods of Proper Cleaning
Proper cleaning requires liquid soap/detergent, water and the use of a clean and disinfected scrub brush to remove all visible debris and residue.
All items should be scrubbed with a clean and disinfected scrub brush under running water.
Cleaning is not disinfection; disinfection is an entirely separate step. Different items are cleaned in different ways. This often depends on the item manufacturing material and how the item has been used.
NOTE: the cleaning step must be properly performed before an item can be disinfected. All items must be thoroughly rinsed and dried with clean cloth or paper towels prior to putting them into a disinfectant.

Methods of Proper Disinfecting
After proper cleaning, all reusable implements/tools must be disinfected by complete immersion in an appropriate disinfecting solution (see below, Appropriate Disinfectants).
The item must be completely immersed so that all surfaces, including handles, are soaked for the time required on the disinfectant manufacturer's label.
In general, U.S. Environmental Protection Agency (EPA) registered disinfectants require 10 minute immersion; isopropyl and ethyl alcohol require 5 minutes.
Remove items after the required time, using clean and disinfected tongs or gloves to avoid skin contact with the disinfectant solution.
If required by the instruction label, rinse thoroughly under running water.
Allow items to air-dry completely by placing them on top of a clean towel and covering them with another clean towel.
Thick foam cushioned buffers should have the moisture pressed out while in between disinfectant products are designed to destroy disease-causing microorganisms (pathogens) on non-living surfaces, such as those described in this document.
They are not appropriate for use on living skin. Contact with skin should be avoided.

Appropriate salon disinfectants include the following:
(a) EPA-registered Hospital disinfectants with bactericidal, fungicidal and virucidal claims on the label.
(b) 10% bleach solution (1 part bleach to 9 parts water)
(c) Isopropyl alcohol, 70%-90% solution
(d) Ethyl alcohol, 70%-90% solution

Individual Client Packs
Tools/instruments kept in individual packs must be properly cleaned and disinfected after each use. If a client provides their own implements/tools, they must be properly cleaned and disinfected before use. State rules require all tools and equipment to be disinfected before being reused, even if used by the same client! Improperly cleaned and disinfected implements may grow infection/disease-causing organisms before the client returns for their next visit, thereby increasing the risk of infection. Never use air-tight bags or containers for storage as these can promote bacterial growth.

Methods for Proper Storage of Tools and Equipment
All properly cleaned, disinfected and dried implements/ tools must be stored in a sanitary manner. A lined drawer is usually adequate, provided it is clean, contains only clean items and is properly labelled. Store soiled or used items in a properly labelled, covered container separate from clean items. Never use airtight containers or zipper bags – these may promote bacterial growth!
Abrasive Files, Buffers and Electric File Bits: after each use abrasive files, buffers, blocks or bits must be thoroughly cleaned by manually brushing with a clean and disinfected brush or by other adequate methods to remove all visible debris. The sides of foam cushioned buffers, blocks or other abrasives should also be brushed after each use. After proper cleaning abrasives files, buffers and blocks are best disinfected by immersing in (or saturating with) 70-90% isopropyl or ethyl alcohol for 5 minutes. Once electric bits have been thoroughly cleaned, they must be disinfected by complete immersion in an appropriate EPA registered disinfectant, as described in the next section. Any porous (absorbent) abrasive file, buffer, block, band, etc. that comes in contact with broken, damaged, infected or unhealthy skin or nails must be properly disposed of immediately, as described below.

Contact with Blood, Body Fluid or Unhealthy Conditions
If blood or body fluid comes in contact with any salon surface, the nail professional should put on a pair of clean protective, disposable gloves and use an EPA-registered Hospital liquid disinfectant or a 10% bleach solution to clean up all visible blood or body fluid. In case of an accidental cut, clean with an antiseptic and bandage the cut. Disposable items, such as a cotton-tipped wood stick must be immediately double-bagged and discarded after use, as described at the end of this section. Any non-porous instrument or implement that comes in contact with an unhealthy condition of the nail or skin, blood or body fluid, must be immediately and properly cleaned, then disinfected using an EPA-registered Hospital disinfectant as directed or a 10% bleach solution for 5 minutes. Any porous/ absorbent instrument that comes in contact with an unhealthy condition of the nail or skin, blood or body fluid must be immediately double-bagged and discarded in a closed trash container or biohazard box.

GIMA WARRANTY CONDITIONS
Congratulations for purchasing a GIMA product.
This product meets high qualitative standards both as regards the material and the production. The warranty is valid for 12 months from the date of supply of GIMA.
During the period of validity of the warranty, GIMA will repair and/or replace free of charge all the defected parts due to production reasons. Labor costs and personnel traveling expenses and packaging not included.
All components subject to wear are not included in the warranty.
The repair or replacement performed during the warranty period shall not extend the warranty.
The warranty is void in the following cases: repairs performed by unauthorized personnel or with non-original spare parts, defects caused by negligence or incorrect use.
GIMA cannot be held responsible for malfunctioning on electronic devices or software due to outside agents such as: voltage changes, electro-magnetic fields, radio interferences, etc.
The warranty is void if the above regulations are not observed and if the serial code (if available) has been removed, cancelled or changed.
The defected products must be returned only to the dealer the product was purchased from. Products sent to GIMA will be rejected.

REF	Codice prodotto Product code Código produto Code produit Erzeugniscode Código producto	LOT	Numero di lotto Lot number Numéro de lot Número de lote Chargennummer Número de lote		Conservare al riparo dalla luce solare Keep away from sunlight Guardar ao abrigo da luz solar Á conserver à l'abri de la lumière du soleil Vor Sonneneinstrahlung geschützt lagern Conservar al amparo de la luz solar		Leggere e seguire attentamente le istruzioni per l'uso Read instructions carefully Ler e seguir atentamente as instruções de uso Lire et suivre attentivement la notice Gebrauchsanweisung sorgfältig lesen und befolgen Leer y seguir atentamente las instrucciones de uso		Non sterile Non-sterile Não estéril Non stérile Nicht steril No estéril
	Fabbricante Manufacturer Fabricante Fabricant Hersteller Fabricante		Leggere attentamente le istruzioni per l'uso Please read instructions carefully Ler atentamente as instruções de uso Lire attentivement la notice Gebrauchsanweisung sorgfältig lesen Leer atentamente las instrucciones de uso		Conservare in luogo fresco ed asciutto Keep in a cool, dry place Armazenar em local fresco e seco Á conserver dans un endroit frais et sec An einem kühlen und trockenen Ort lagern Conservar en un lugar fresco y seco		Prodotto conforme alla Direttiva Europea Product complies with European Directive Produto em conformidade com a Diretiva Europeia Ce produit est conforme à la directive européenne Produkt gemäß EU-Richtlinie Producto conforme a la Directiva Europea		